


NOTES:

- 1.) FOR INSTRUMENT INSTALLATION DETAILS SEE PSI DWG. #V049-3-008.
- 2.) ALL INSTRUMENT AIR & PROCESS TUBING SHALL BE 3/8" O.D. x .049 THK SEAMLESS SSTL TYPE 316.
- 3.) TUBING ROUTING SHOWN ON PLAN IS DIAGRAMMATICAL AND SHALL BE FIELD VERIFIED SO AS TO OPTIMIZE SUPPORTING MEANS AND TO AVOID INTERFERENCES WITH CONDUIT & PIPING SYSTEMS.

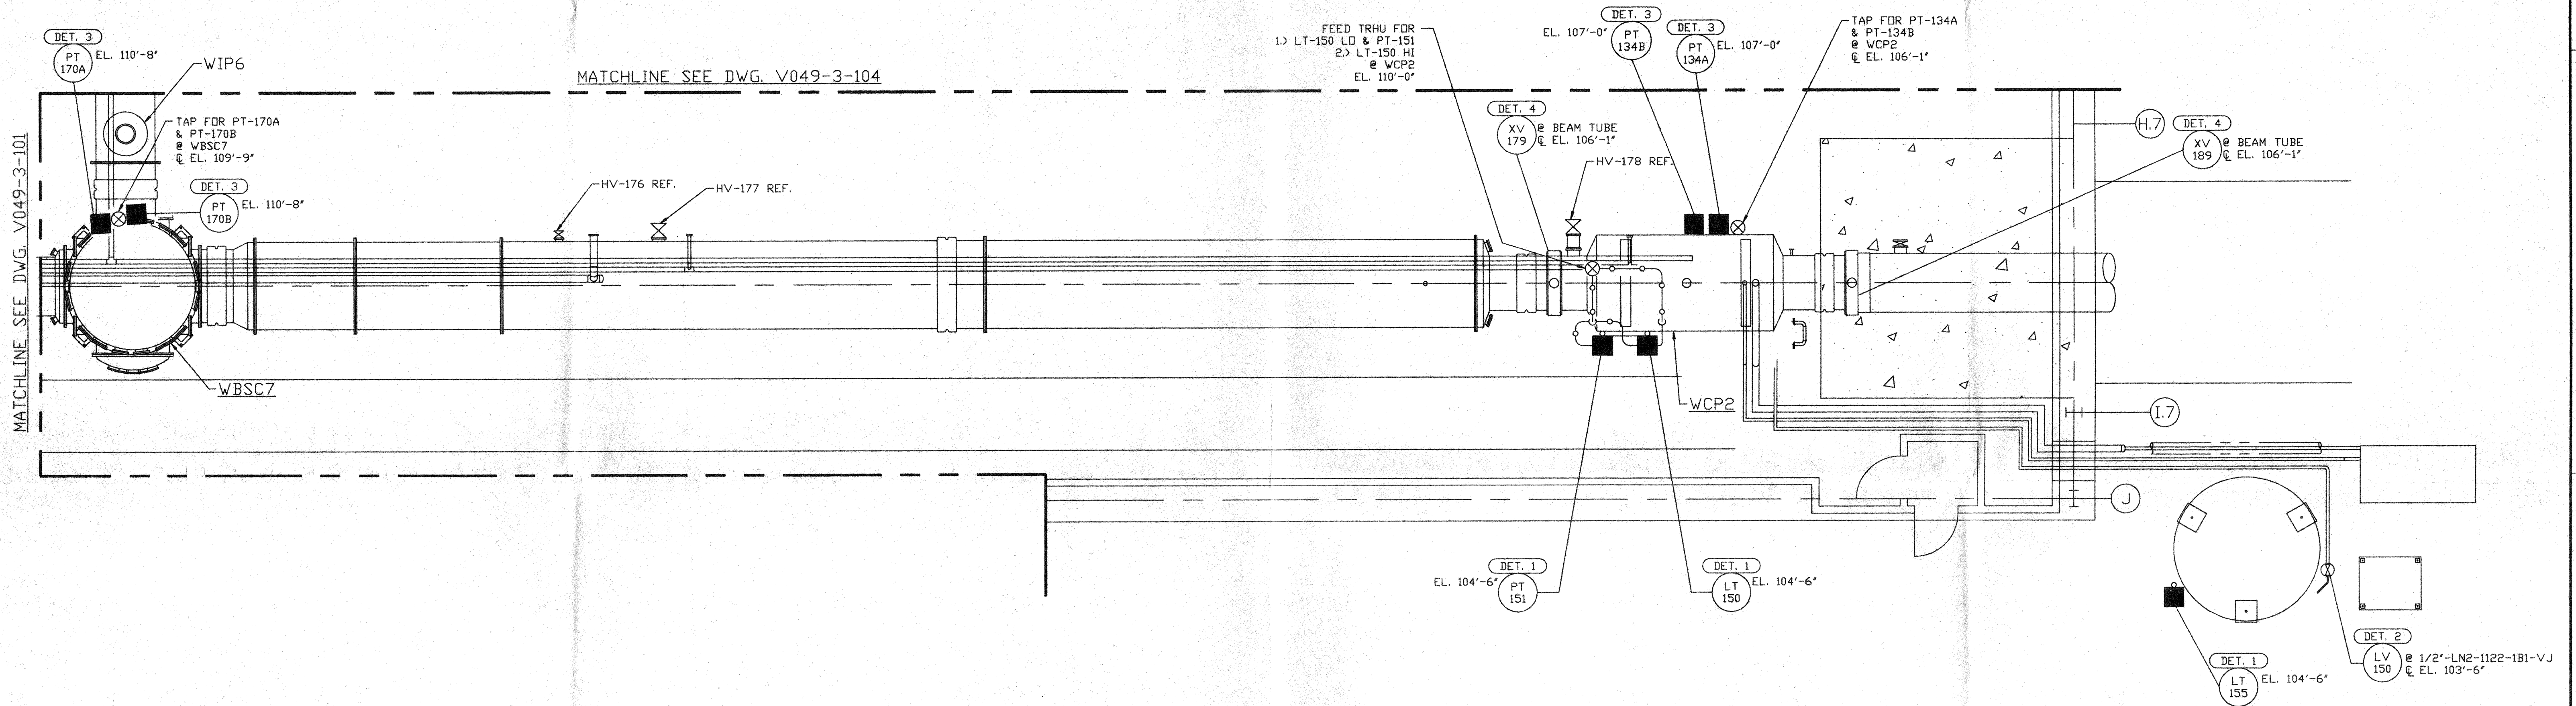

INSTRUMENTS NOT LOCATED	
TE 152	
TE 153A	
TE 153B	TE 153C
TY 153	
FE 154	
F1 154	
PCV 170	
INSTRUMENT AIR	

NOT FOR CONSTRUCTION

LEGEND

- INSTRUMENT LOCATION
 - XX INSTRUMENT IDENTIFICATION
 - DET. X INSTALLATION DETAIL SEE NOTE 1
 - ⊗ PROCESS TAP
 - PROCESS TUBING (SEE NOTE 2)
 - #— INSTRUMENT AIR (SEE NOTE 2)
- APR 30 1998

D960551-00-V

PROPRIETARY AND CONFIDENTIAL		UNLESS OTHERWISE SPECIFIED DIMENSIONS ARE IN INCHES										PROCESS SYSTEMS INTERNATIONAL INC. 20 WALKUP DR. WESTBOROUGH, MASSACHUSETTS 01581 USA	
THIS DOCUMENT CONTAINS PROPRIETARY INFORMATION BELONGING TO PROCESS SYSTEMS INTERNATIONAL, INC. OR ITS AFFILIATED COMPANIES AND SHALL BE USED ONLY FOR THE PURPOSE FOR WHICH IT WAS SUPPLIED. IT SHALL NOT BE COPIED, REPRODUCED OR OTHERWISE USED, NOR SHALL SUCH INFORMATION BE FURNISHED IN WHOLE OR IN PART TO OTHERS EXCEPT IN ACCORDANCE WITH THE TERMS OF ANY AGREEMENT UNDER WHICH IT WAS SUPPLIED OR WITH THE PRIOR WRITTEN CONSENT OF PROCESS SYSTEMS INTERNATIONAL, INC. AND SHALL BE RETURNED UPON REQUEST.		TOLERANCES:										INSTRUMENT PLAN LIGO VACUUM EQUIPMENT WASHINGTON SITE RIGHT BEAM MANIFOLD	
V049-3-104	INSTRUMENT PLAN DIAGONAL SECTION		FRACTIONAL ±										CAD FILE
V049-3-101	INSTRUMENT PLAN VERTEX SECTION		ANGULAR/RADIUS 40°-30° BEND 42°										SIZE
V049-3-008	INSTRUMENT INSTALLATION DETAILS		TWO PLACE DECIMAL ± .01										DWG. NO.
V049-3-002	WASHINGTON OVERALL SITE PLAN		THREE PLACE DECIMAL ± .005										V049-3-103
V049-3-001	GENERAL NOTES & LEGEND		FINISHED SURFACE, RMS										REV.
V049-0-015	P & I D WASHINGTON RIGHT BEAM MANIFOLD	V049-5-001	BREAK CORNERS IN OUT.										0
DWG. NO.	DESCRIPTION	DWG. NO.	REMOVE ALL BURRS	DO NOT SCALE THIS DRAWING	0	ISSUE FOR FDR							SCALE
				USED ON:	REV.	DESCRIPTION							3/16" = 1' - 0"
				NEXT ASS'Y:									SHEET
													1 OF 1