

---

# LHOY-End RxPD and TxPD Calibration Trends

## Table of Contents

About .....	1
WS/TX Ratio when WS is at TX (Inner Beam) .....	2
WS/TX Ratio when WS is at TX (Outer Beam) .....	3
WS/TX Ratio when WS is at RX (Inner Beam) .....	4
WS/TX Ratio when WS is at RX (Outer Beam) .....	5
RX/TX Ratio (Inner Beam) .....	6
RX/TX Ratio (Outer Beam) .....	7
Optical Efficiency of Inner Beam .....	8
Optical Efficiency of Outer Beam .....	9
Total Optical Efficiency .....	11
TX/WS Ratio .....	12
RX/WS Ratio .....	13
TX/WS Ratio (Corrected for OE) .....	14
RX/WS Ratio (Corrected for OE) .....	15
Power Imbalance .....	16
Summary .....	17

## About

This document contains the Pcal PD (TxPD and RxPD) Calibration trends. The first six sections contain the six ratios measured at the end-station labeled as m1, m2 .....m6. The section that follows contains the relevant information calculated from these measurements which include Optical Efficiency, Power Imbalance, TX/WS and RX/WS ratio.

### Understanding Each Section

Each section contains a list of measurements with Magnitude, Standard Error (Std Err) and Relative Error (Rel Err) for each measurement. The list is followed by two plot figures with Magnitude on the first plot and the the Normalized Magnitude on the second. Each section ends with a summary that contains the weighted mean of all the measurement along with their Standard Deviation (Std Dev), Std Err and Rel Err where each of


$$\begin{aligned} \text{Mean} &= \text{sum}(x(i)*w(i))/\text{sum}(w(i)) \\ \text{Std Dev} &= \text{sqrt}(\text{sum}(w(i)*(x(i)-x\_mean)^2)/((n-1)/n*\text{sum}(w(i)))) \\ \text{Std Err} &= \text{Std Dev}/\text{sqrt}(n) \\ \text{Rel Err} &= \text{Std Err}/\text{Mean} \end{aligned}$$

*Report created on 11-Oct-2016*

# WS/TX Ratio when WS is at TX (Inner Beam)

## List of Measurements

<i>Date</i>	<i><math>m1 \pm SE_{\{m1\}}</math></i>	<i>Normalized</i>
D20150811	$-0.180846 \pm 0.000008$	$(1 \pm 0.000044)$
D20150827	$-0.180614 \pm 0.000007$	$(1 \pm 0.000037)$
D20151013	$-0.180474 \pm 0.000006$	$(1 \pm 0.000034)$
D20151222	$-0.180696 \pm 0.000008$	$(1 \pm 0.000044)$
D20160505	$-0.178817 \pm 0.000008$	$(1 \pm 0.000043)$
D20160628	$-0.178884 \pm 0.000007$	$(1 \pm 0.000041)$
D20160927	$-0.179158 \pm 0.000008$	$(1 \pm 0.000046)$
D20161011	$-0.179883 \pm 0.000010$	$(1 \pm 0.000054)$

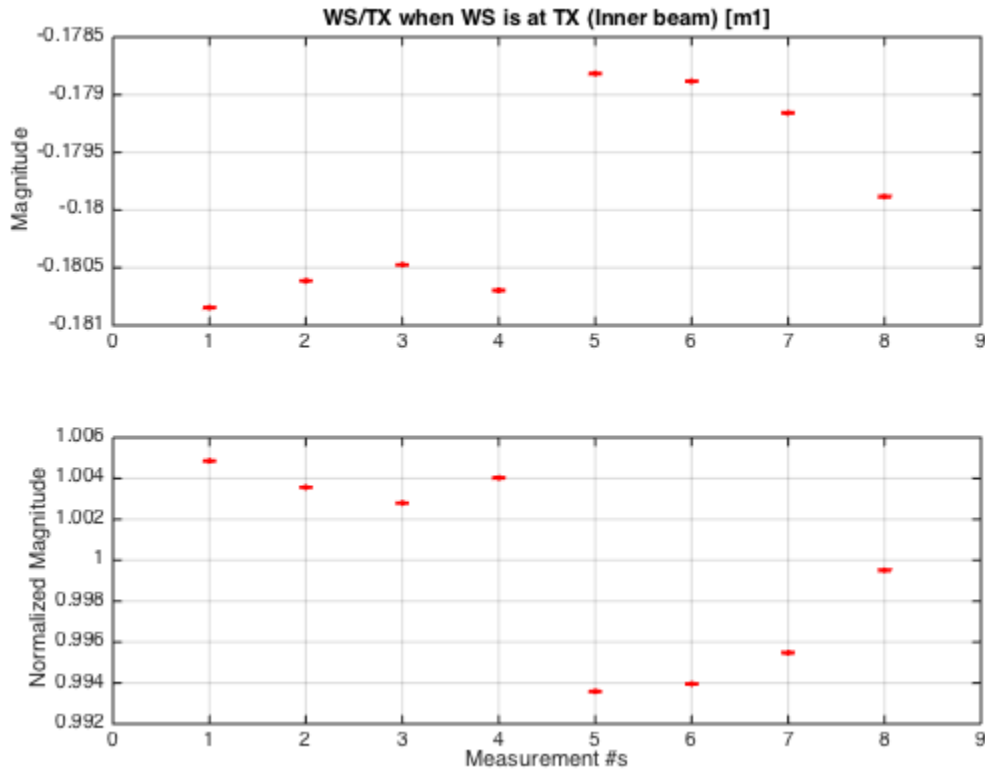



Summary of WS/TX when WS is at TX (Inner beam) [m1]:  
Mean value:  $-0.179972$   
Standard deviation:  $0.000856$

Standard Error: 0.000323  
Relative Standard Error: 0.001793

## WS/TX Ratio when WS is at TX (Outer Beam)

### List of Measurements

Date	$m2 \pm SE_{\{m2\}}$	Normalized
D20150811	$-0.183815 \pm 0.000007$	$(1 \pm 0.000039)$
D20150827	$-0.183788 \pm 0.000006$	$(1 \pm 0.000035)$
D20151013	$-0.184127 \pm 0.000007$	$(1 \pm 0.000036)$
D20151222	$-0.184502 \pm 0.000005$	$(1 \pm 0.000027)$
D20160505	$-0.183087 \pm 0.000008$	$(1 \pm 0.000044)$
D20160628	$-0.183461 \pm 0.000008$	$(1 \pm 0.000042)$
D20160927	$-0.184007 \pm 0.000008$	$(1 \pm 0.000044)$
D20161011	$-0.181887 \pm 0.000010$	$(1 \pm 0.000053)$

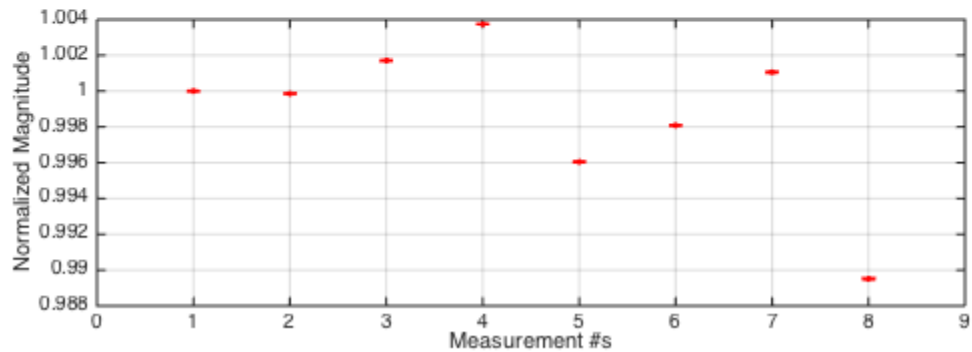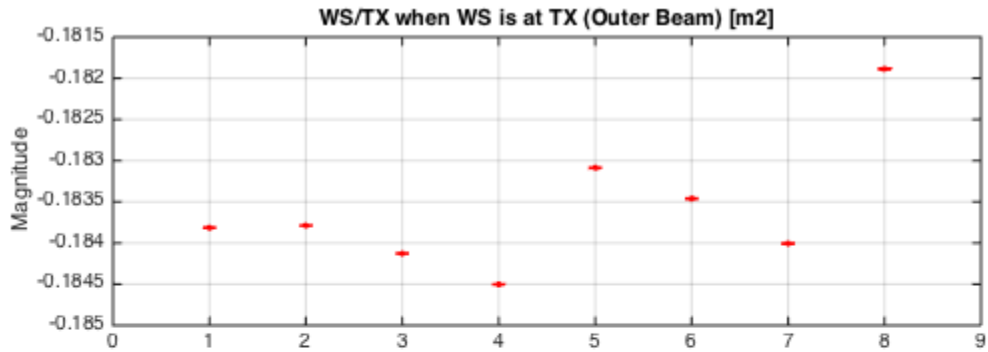

LHOY-End RxPD and Tx-  
PD Calibration Trends

---


Summary of WS/TX when WS is at TX (Outer Beam) [m2]:

Mean value: -0.183814  
Standard deviation: 0.000708  
Standard Error: 0.000267  
Relative Standard Error: 0.001453

## WS/TX Ratio when WS is at RX (Inner Beam)

### List of Measurements

<i>Date</i>	<i>m3 ± SE_{m3}</i>	<i>Normalized</i>
D20150811	-0.179002 ± 0.000008	(1 ± 0.000043)
D20150827	-0.176861 ± 0.000006	(1 ± 0.000036)
D20151013	-0.178931 ± 0.000006	(1 ± 0.000035)
D20151222	-0.179098 ± 0.000007	(1 ± 0.000037)
D20160505	-0.177402 ± 0.000008	(1 ± 0.000043)
D20160628	-0.177210 ± 0.000008	(1 ± 0.000043)
D20160927	-0.178050 ± 0.000008	(1 ± 0.000046)
D20161011	-0.177663 ± 0.000009	(1 ± 0.000050)

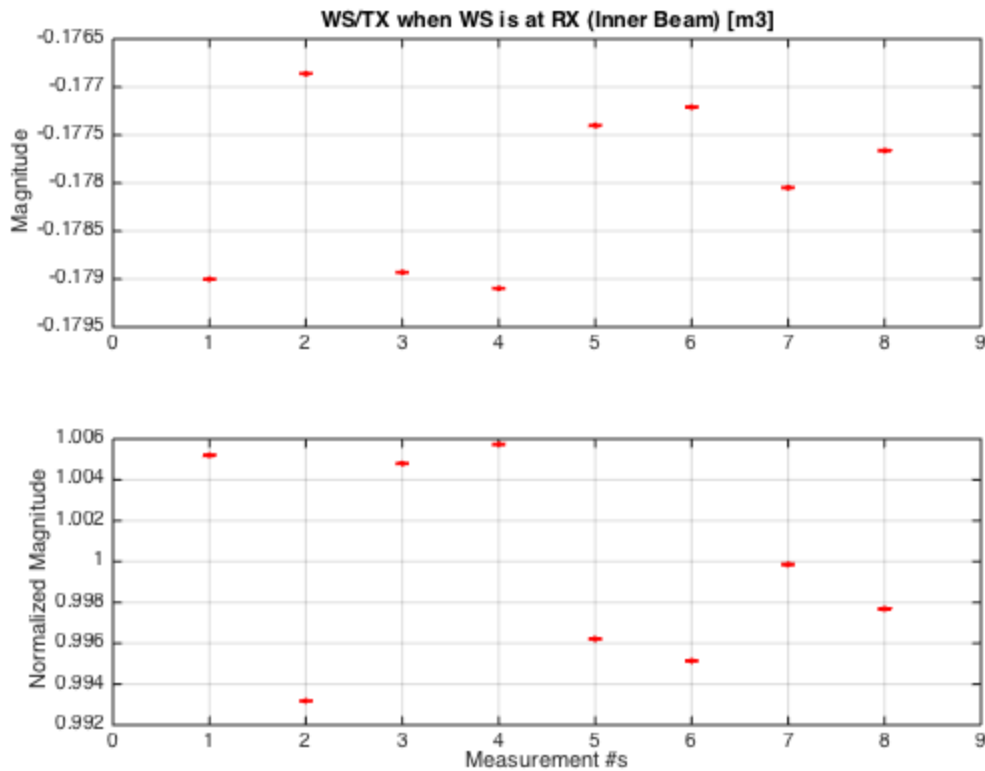


Summary of WS/TX when WS is at RX (Inner Beam) [m3]:  
 Mean value: -0.178076  
 Standard deviation: 0.000934  
 Standard Error: 0.000352  
 Relative Standard Error: 0.001977

## WS/TX Ratio when WS is at RX (Outer Beam)

### List of Measurements

Date	$m4 \pm SE_{\{m4\}}$	Normalized
D20150811	$-0.181381 \pm 0.000008$	$(1 \pm 0.000046)$
D20150827	$-0.181640 \pm 0.000006$	$(1 \pm 0.000031)$
D20151013	$-0.181781 \pm 0.000006$	$(1 \pm 0.000034)$
D20151222	$-0.182083 \pm 0.000006$	$(1 \pm 0.000031)$
D20160505	$-0.180668 \pm 0.000007$	$(1 \pm 0.000040)$
D20160628	$-0.180940 \pm 0.000007$	$(1 \pm 0.000040)$
D20160927	$-0.182118 \pm 0.000009$	$(1 \pm 0.000048)$

D20161011       $-0.179869 \pm 0.000008$        $(1 \pm 0.000046)$

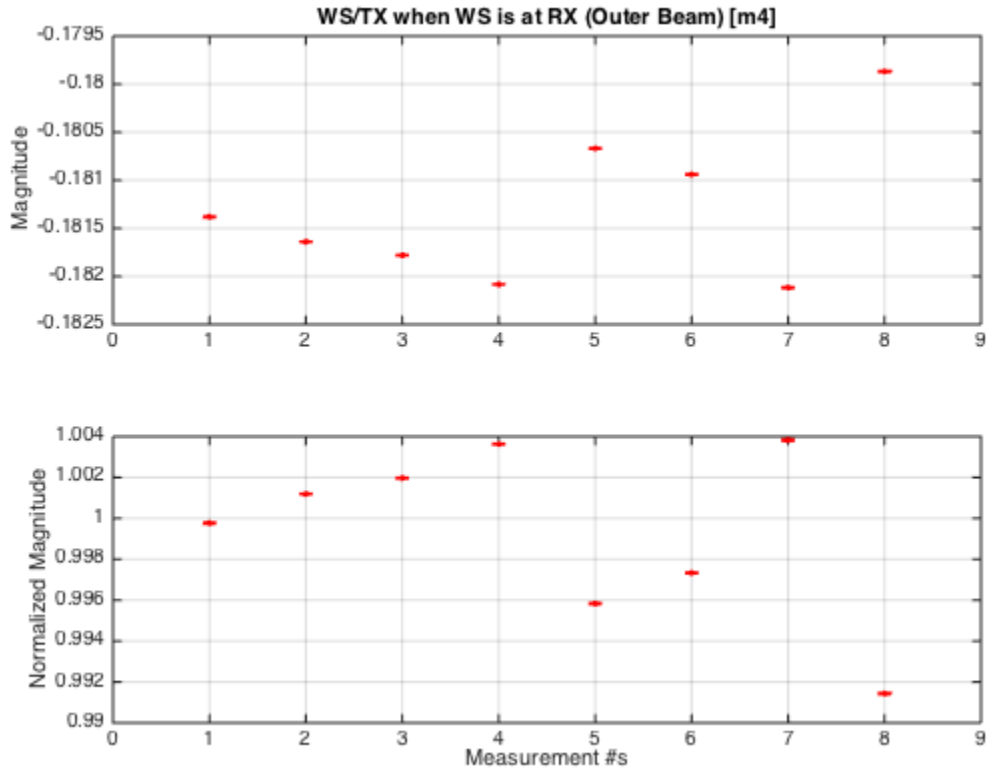

Summary of WS/TX when WS is at RX (Outer Beam) [m4]:  
 Mean value:       $-0.181424$   
 Standard deviation:       $0.000709$   
 Standard Error:       $0.000267$   
 Relative Standard Error:       $0.001474$

## RX/TX Ratio (Inner Beam)


### List of Measurements

Date	$m5 \pm SE_{\{m5\}}$	Normalized
D20150811	$0.716408 \pm 0.000003$	$(1 \pm 0.000005)$
D20150827	$0.715858 \pm 0.000003$	$(1 \pm 0.000004)$
D20151013	$0.715399 \pm 0.000002$	$(1 \pm 0.000003)$
D20151222	$0.716771 \pm 0.000002$	$(1 \pm 0.000003)$
D20160505	$0.717343 \pm 0.000002$	$(1 \pm 0.000003)$

LHOY-End RxPD and Tx-  
PD Calibration Trends

---

D20160628	$0.715799 \pm 0.000002$	$(1 \pm 0.000003)$
D20160927	$0.715156 \pm 0.000003$	$(1 \pm 0.000004)$
D20161011	$0.715926 \pm 0.000004$	$(1 \pm 0.000006)$

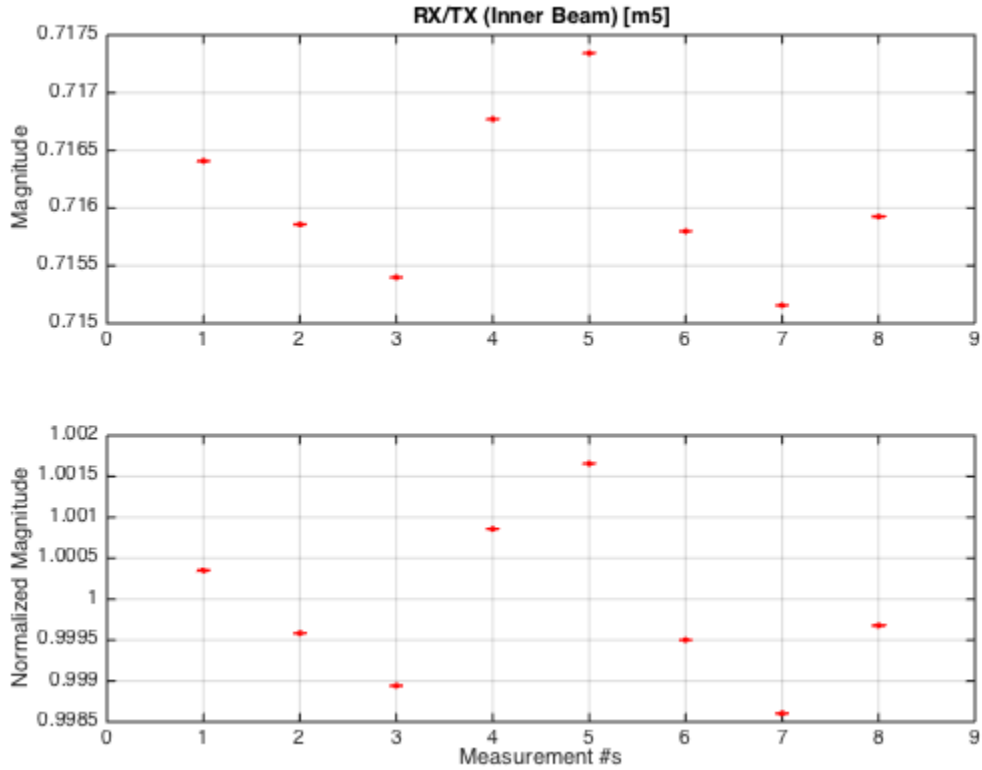

Summary of RX/TX (Inner Beam) [m5]:

Mean value:	0.716157
Standard deviation:	0.000788
Standard Error:	0.000297
Relative Standard Error:	0.000415

## RX/TX Ratio (Outer Beam)


### List of Measurements

Date	$m6 \pm SE_{\{m6\}}$	Normalized
D20150811	$0.726657 \pm 0.000003$	$(1 \pm 0.000004)$
D20150827	$0.726468 \pm 0.000002$	$(1 \pm 0.000003)$
D20151013	$0.727582 \pm 0.000002$	$(1 \pm 0.000003)$

LHOY-End RxPD and Tx-  
PD Calibration Trends

---

<i>D20151222</i>	$0.728972 \pm 0.000002$	$(1 \pm 0.000003)$
<i>D20160505</i>	$0.730960 \pm 0.000002$	$(1 \pm 0.000003)$
<i>D20160628</i>	$0.732089 \pm 0.000003$	$(1 \pm 0.000004)$
<i>D20160927</i>	$0.732393 \pm 0.000002$	$(1 \pm 0.000003)$
<i>D20161011</i>	$0.726292 \pm 0.000003$	$(1 \pm 0.000004)$

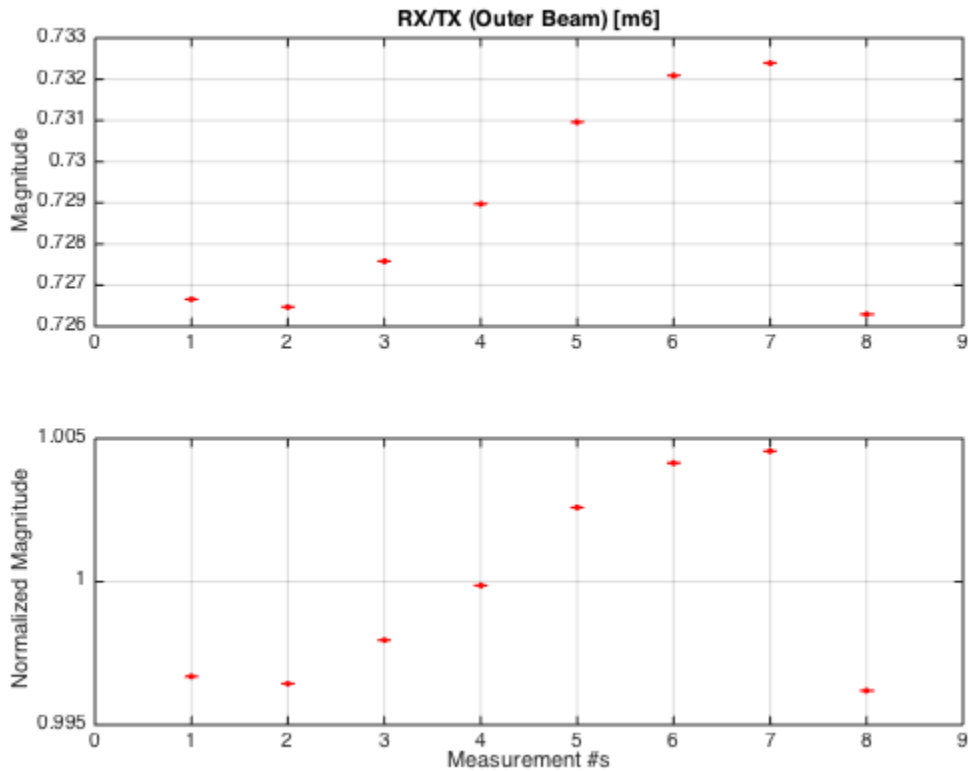

*Summary of RX/TX (Outer Beam) [m6]:*

<i>Mean value:</i>	$0.729068$
<i>Standard deviation:</i>	$0.002444$
<i>Standard Error:</i>	$0.000922$
<i>Relative Standard Error:</i>	$0.001264$

## Optical Efficiency of Inner Beam


### List of Measurements

<i>Date</i>	$e_i \pm SE_{\{e_i\}}$	<i>Normalized</i>
<i>D20150811</i>	$0.989808 \pm 0.000062$	$(1 \pm 0.000062)$



LHOY-End RxPD and Tx-  
PD Calibration Trends

D20150827	0.979224 ± 0.000052	(1 ± 0.000053)
D20151013	0.991448 ± 0.000049	(1 ± 0.000049)
D20151222	0.991154 ± 0.000057	(1 ± 0.000058)
D20160505	0.992086 ± 0.000061	(1 ± 0.000061)
D20160628	0.990643 ± 0.000059	(1 ± 0.000060)
D20160927	0.993815 ± 0.000065	(1 ± 0.000065)
D20161011	0.987658 ± 0.000074	(1 ± 0.000075)

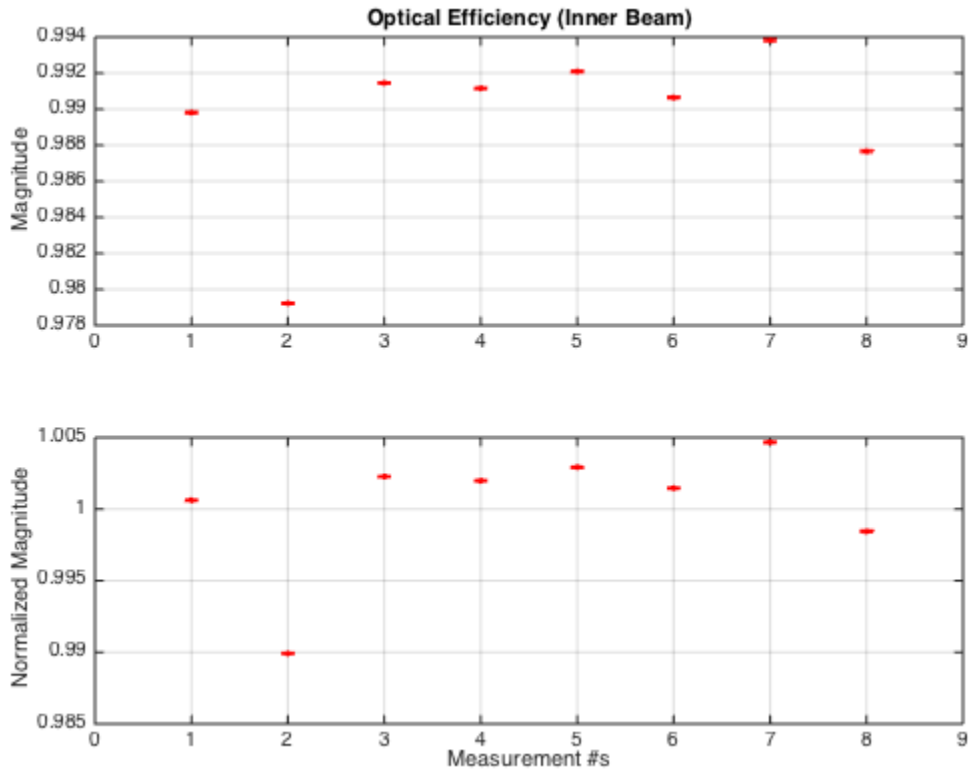

Summary of Optical Efficiency (Inner Beam):


Mean value: 0.989196  
Standard deviation: 0.004884  
Standard Error: 0.001842  
Relative Standard Error: 0.001862

## Optical Efficiency of Outer Beam

List of Measurements

LHOY-End RxPD and Tx-  
PD Calibration Trends

<i>Date</i>	<i>e<sub>o</sub> ± SE_{e<sub>o</sub>}</i>	<i>Normalized</i>
D20150811	0.986759 ± 0.000061	(1 ± 0.000062)
D20150827	0.988317 ± 0.000047	(1 ± 0.000047)
D20151013	0.987256 ± 0.000049	(1 ± 0.000050)
D20151222	0.986890 ± 0.000041	(1 ± 0.000041)
D20160505	0.986788 ± 0.000060	(1 ± 0.000061)
D20160628	0.986257 ± 0.000058	(1 ± 0.000059)
D20160927	0.989731 ± 0.000065	(1 ± 0.000066)
D20161011	0.988909 ± 0.000070	(1 ± 0.000071)

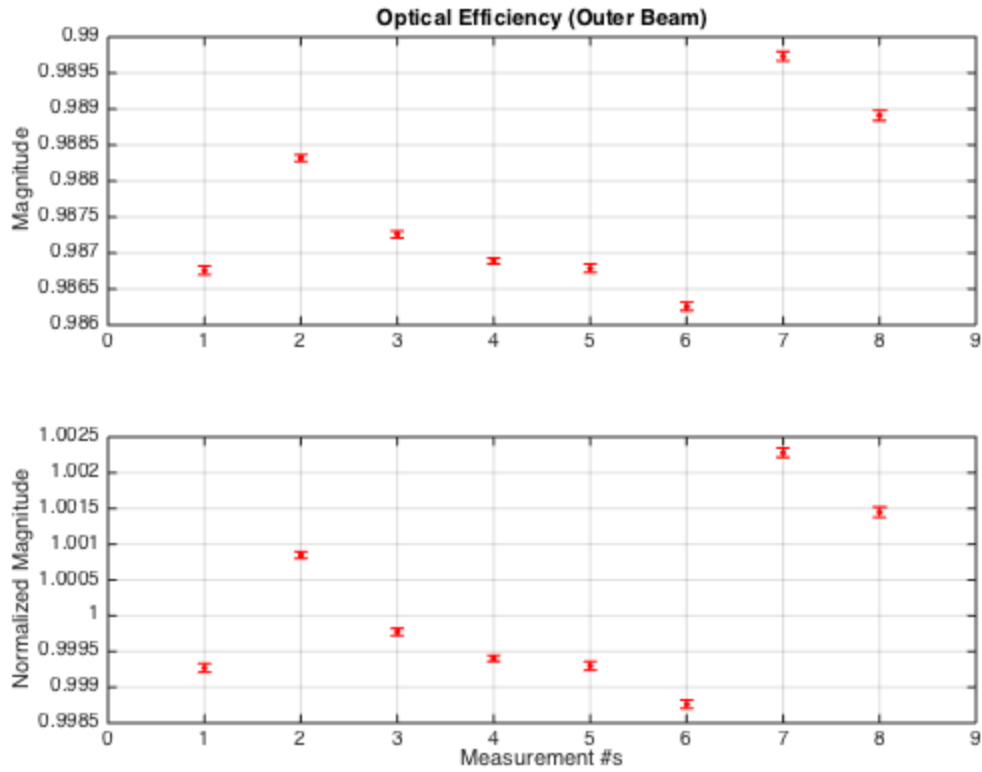


*Summary of Optical Efficiency (Outer Beam):*

*Mean value:*           0.987480  
*Standard deviation:*   0.001090  
*Standard Error:*       0.000411  
*Relative Standard Error:* 0.000416

# Total Optical Efficiency

## List of Measurements

Date	$e \pm SE_{\{e\}}$	Normalized
D20150811	$0.988271 \pm 0.000043$	$(1 \pm 0.000043)$
D20150827	$0.983810 \pm 0.000034$	$(1 \pm 0.000035)$
D20151013	$0.989331 \pm 0.000034$	$(1 \pm 0.000035)$
D20151222	$0.989000 \pm 0.000035$	$(1 \pm 0.000035)$
D20160505	$0.989405 \pm 0.000042$	$(1 \pm 0.000043)$
D20160628	$0.988423 \pm 0.000041$	$(1 \pm 0.000041)$
D20160927	$0.991746 \pm 0.000046$	$(1 \pm 0.000046)$
D20161011	$0.988287 \pm 0.000050$	$(1 \pm 0.000051)$

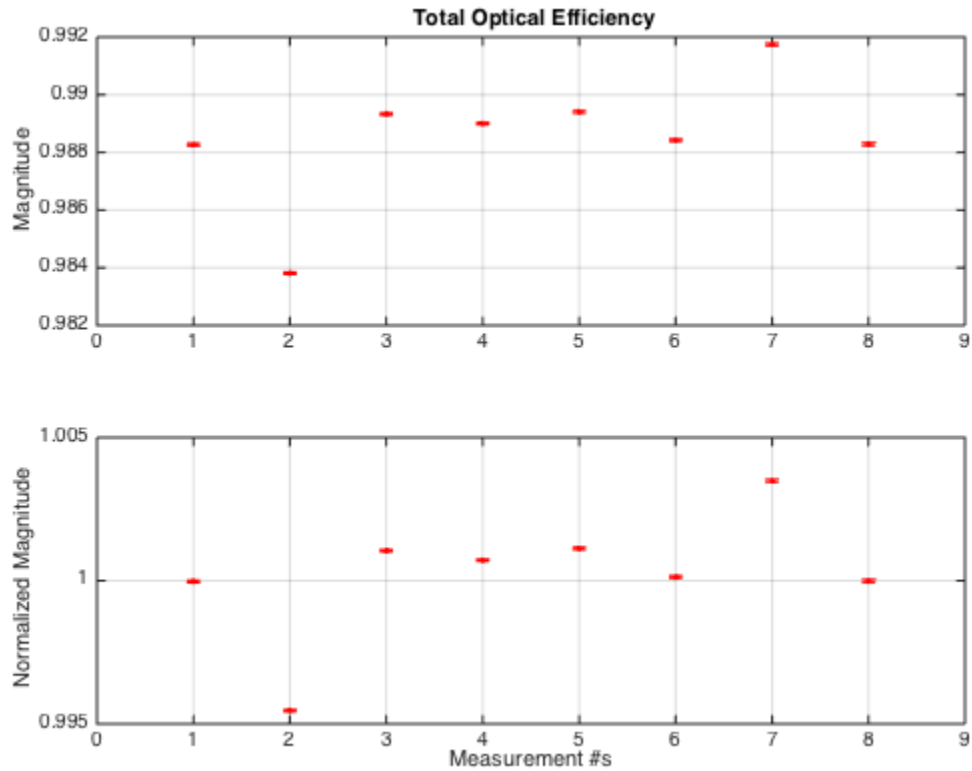

Summary of Total Optical Efficiency:

Mean value: 0.988294  
Standard deviation: 0.002358


LHOY-End RxPD and Tx-  
PD Calibration Trends

Standard Error: 0.000889  
Relative Standard Error: 0.000900

# TX/WS Ratio

## List of Measurements

Date	$R_{TW} \pm SE_{\{R_{TW}\}}$	Normalized
D20150811	$-2.742279 \pm 0.000011$	$(1 \pm 0.000004)$
D20150827	$-2.744228 \pm 0.000009$	$(1 \pm 0.000003)$
D20151013	$-2.742723 \pm 0.000009$	$(1 \pm 0.000003)$
D20151222	$-2.738239 \pm 0.000009$	$(1 \pm 0.000003)$
D20160505	$-2.763161 \pm 0.000011$	$(1 \pm 0.000004)$
D20160628	$-2.759803 \pm 0.000011$	$(1 \pm 0.000004)$
D20160927	$-2.753569 \pm 0.000011$	$(1 \pm 0.000004)$
D20161011	$-2.764191 \pm 0.000014$	$(1 \pm 0.000005)$

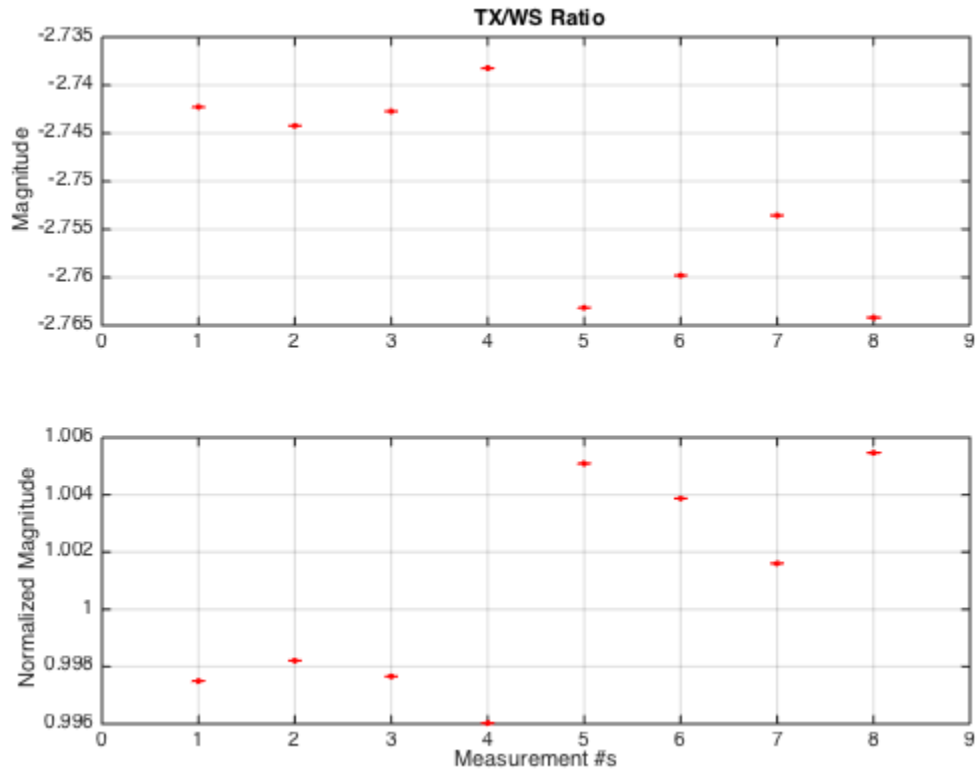

LHOY-End RxPD and Tx-  
PD Calibration Trends

---


Summary of TX/WS Ratio:

Mean value: -2.749164  
Standard deviation: 0.010033  
Standard Error: 0.003783  
Relative Standard Error: 0.001376

## RX/WS Ratio

### List of Measurements

<i>Date</i>	<i>R<sub>RW</sub> ± SE_{R<sub>RW</sub>}</i>	<i>Normalized</i>
D20150811	-4.004239 ± 0.000126	(1 ± 0.000032)
D20150827	-4.023526 ± 0.000096	(1 ± 0.000024)
D20151013	-4.000359 ± 0.000097	(1 ± 0.000024)
D20151222	-4.002816 ± 0.000096	(1 ± 0.000024)
D20160505	-4.044736 ± 0.000119	(1 ± 0.000029)
D20160628	-4.042655 ± 0.000118	(1 ± 0.000029)
D20160927	-4.019073 ± 0.000135	(1 ± 0.000033)
D20161011	-4.033790 ± 0.000139	(1 ± 0.000034)

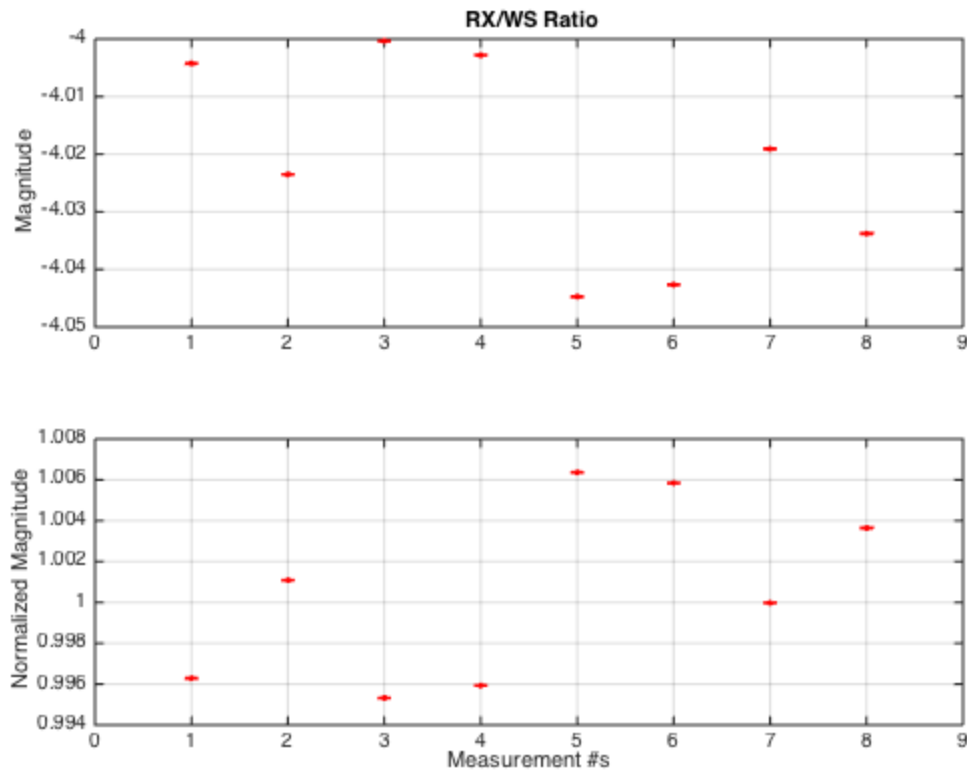

Summary of RX/WS Ratio:

Mean value: -4.019166  
 Standard deviation: 0.017974  
 Standard Error: 0.006777  
 Relative Standard Error: 0.001686


## TX/WS Ratio (Corrected for OE)

### List of Measurements

Date	$R\_TWC \pm SE\{R\_TWC\}$	Normalized
D20150811	-2.758456 ± 0.000060	(1 ± 0.000022)
D20150827	-2.766624 ± 0.000048	(1 ± 0.000017)
D20151013	-2.757433 ± 0.000048	(1 ± 0.000017)
D20151222	-2.753383 ± 0.000048	(1 ± 0.000018)
D20160505	-2.777877 ± 0.000059	(1 ± 0.000021)
D20160628	-2.775872 ± 0.000058	(1 ± 0.000021)
D20160927	-2.764980 ± 0.000064	(1 ± 0.000023)

LHOY-End RxPD and Tx-  
PD Calibration Trends

D20161011                       $-2.780474 \pm 0.000071$                        $(1 \pm 0.000025)$

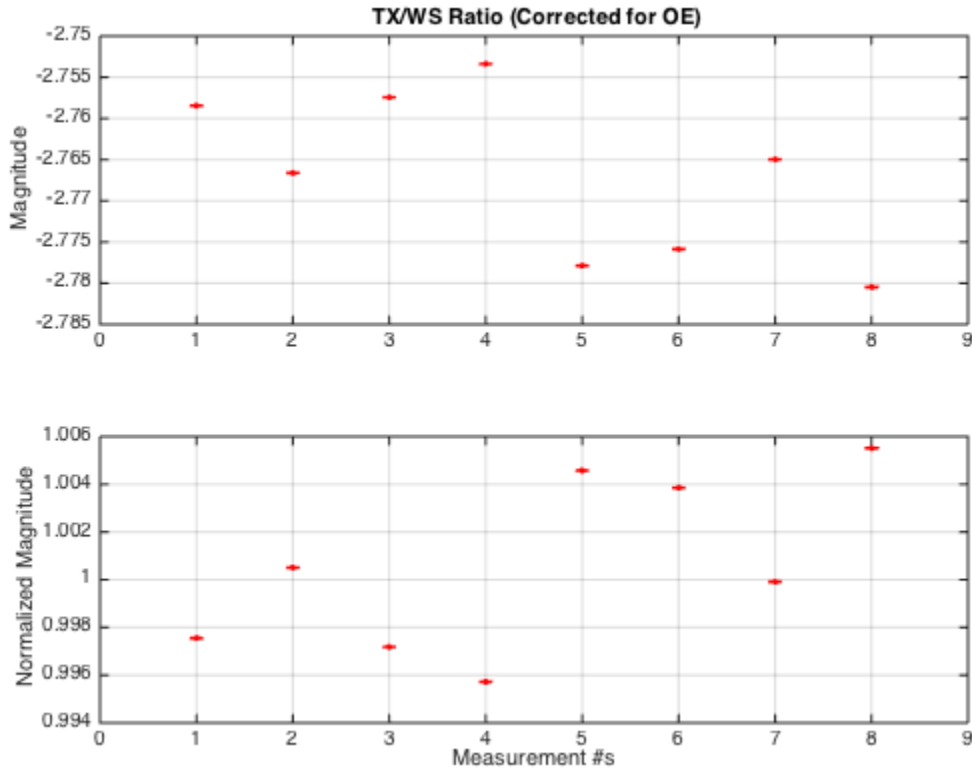

Summary of TX/WS Ratio (Corrected for OE):

Mean value:                       $-2.765224$   
Standard deviation:                       $0.009957$   
Standard Error:                       $0.003754$   
Relative Standard Error:                       $0.001358$

## RX/WS Ratio (Corrected for OE)


### List of Measurements

Date	$R\_Rwc \pm SE_{\{R\_Rwc\}}$	Normalized
D20150811	$-3.980617 \pm 0.000087$	$(1 \pm 0.000022)$
D20150827	$-3.990691 \pm 0.000070$	$(1 \pm 0.000018)$
D20151013	$-3.978905 \pm 0.000069$	$(1 \pm 0.000017)$
D20151222	$-3.980678 \pm 0.000070$	$(1 \pm 0.000018)$
D20160505	$-4.023196 \pm 0.000086$	$(1 \pm 0.000021)$

LHOY-End RxPD and Tx-  
PD Calibration Trends

---

D20160628	$-4.019117 \pm 0.000084$	$(1 \pm 0.000021)$
D20160927	$-4.002417 \pm 0.000092$	$(1 \pm 0.000023)$
D20161011	$-4.010027 \pm 0.000103$	$(1 \pm 0.000026)$

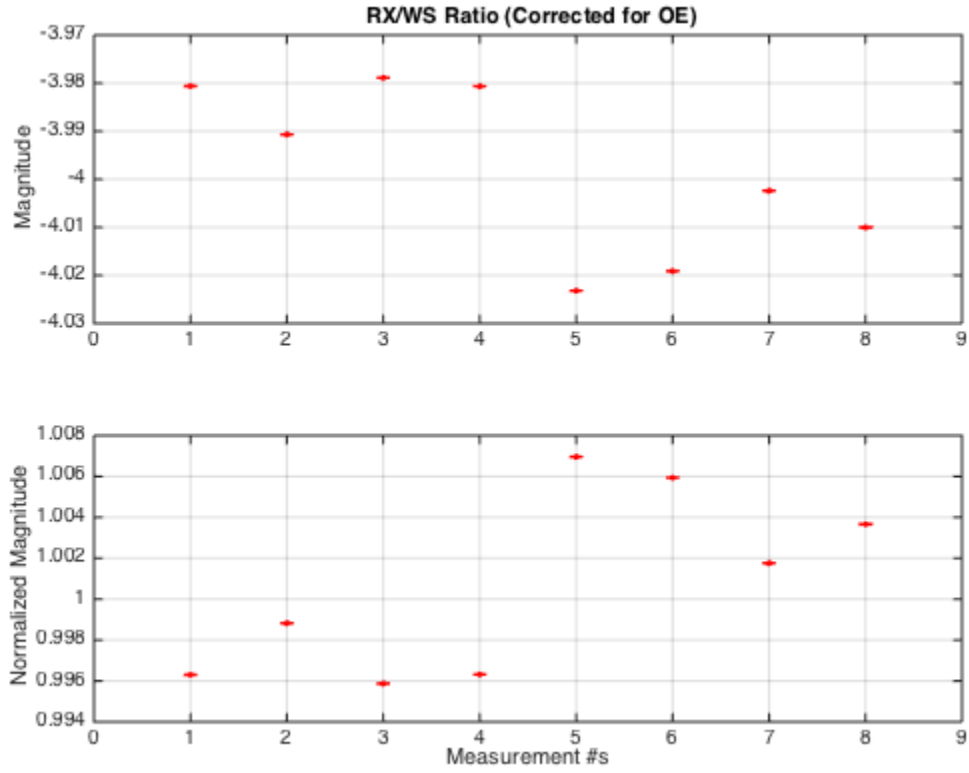

Summary of RX/WS Ratio (Corrected for OE):  
 Mean value:  $-3.995395$   
 Standard deviation:  $0.017853$   
 Standard Error:  $0.006732$   
 Relative Standard Error:  $0.001685$

## Power Imbalance

### List of Measurements


D20150811	$0.983938 \pm 0.000059$	$(1 \pm 0.000059)$
D20150827	$0.982844 \pm 0.000050$	$(1 \pm 0.000051)$
D20151013	$0.980135 \pm 0.000048$	$(1 \pm 0.000049)$
D20151222	$0.979459 \pm 0.000051$	$(1 \pm 0.000052)$



LHOY-End RxPD and Tx-  
PD Calibration Trends

---

D20160505	0.976585 ± 0.000060	(1 ± 0.000062)
D20160628	0.974999 ± 0.000057	(1 ± 0.000059)
D20160927	0.973728 ± 0.000061	(1 ± 0.000063)
D20161011	0.989087 ± 0.000075	(1 ± 0.000075)

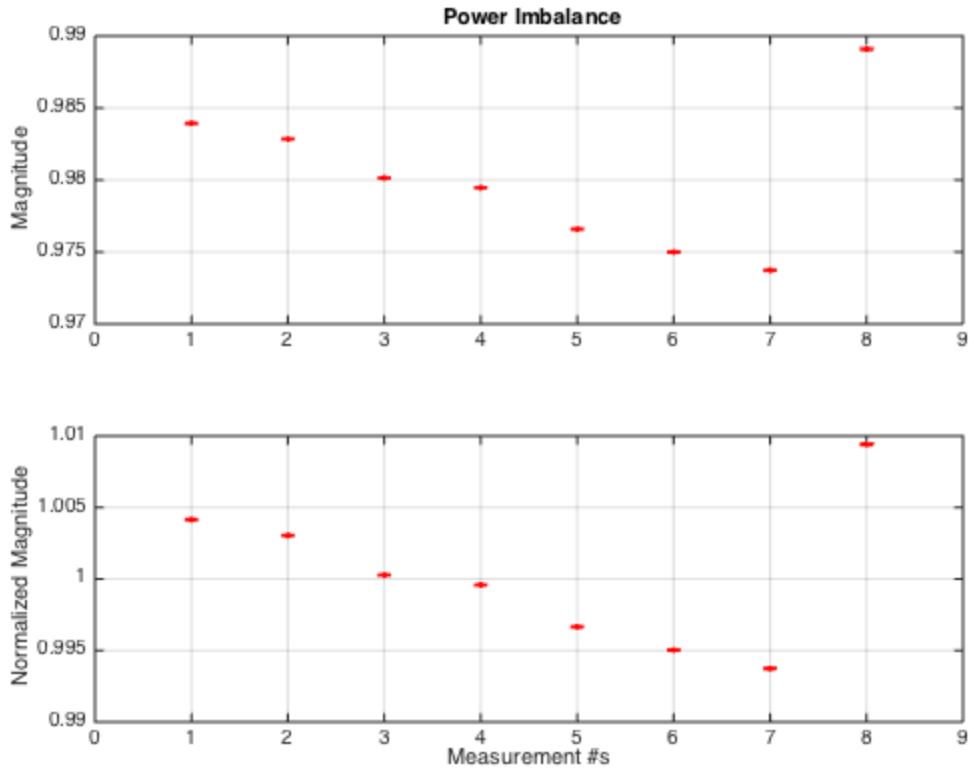

Summary of Power Imbalance:

Mean value:	0.979866
Standard deviation:	0.004451
Standard Error:	0.001678
Relative Standard Error:	0.001713

## Summary

Description	Value	Std Dev	Std Err	Rel Err:
OE (e)	0.9883	0.0024	0.0009	0.0009
TX/WS (a1a2)	-2.7652	0.0100	0.0038	0.0014
RX/WS (b1b2)	-3.9954	0.0179	0.0067	0.0017
W (a5)	1.0000	----	----	0.0034

*Published with MATLAB® R2014b*